


PT-141 HPLC

Test time	:05/07/2018, 09:25	Product Name	:PT-141
Analyst	:LZH	Batch number	:US20180507
Column	:GSA46250BI017013, C18, 4.6*250mm, 5um	Flow Rate	:1.0ml/min
Solvent A	:100% Acetonitrile	Wavelength	:220nm
Solvent B	:0.1% Trifluoroacetic in 100% Water	Temperature	:37°C
Gradient	:	Concentration	:1mg/ml
	A B	Sample Volume	:10ul
	0.0min 5% 95%		
	25.0min 95% 5%		
	25.1min 100% 0%		
	30.0min Stop		

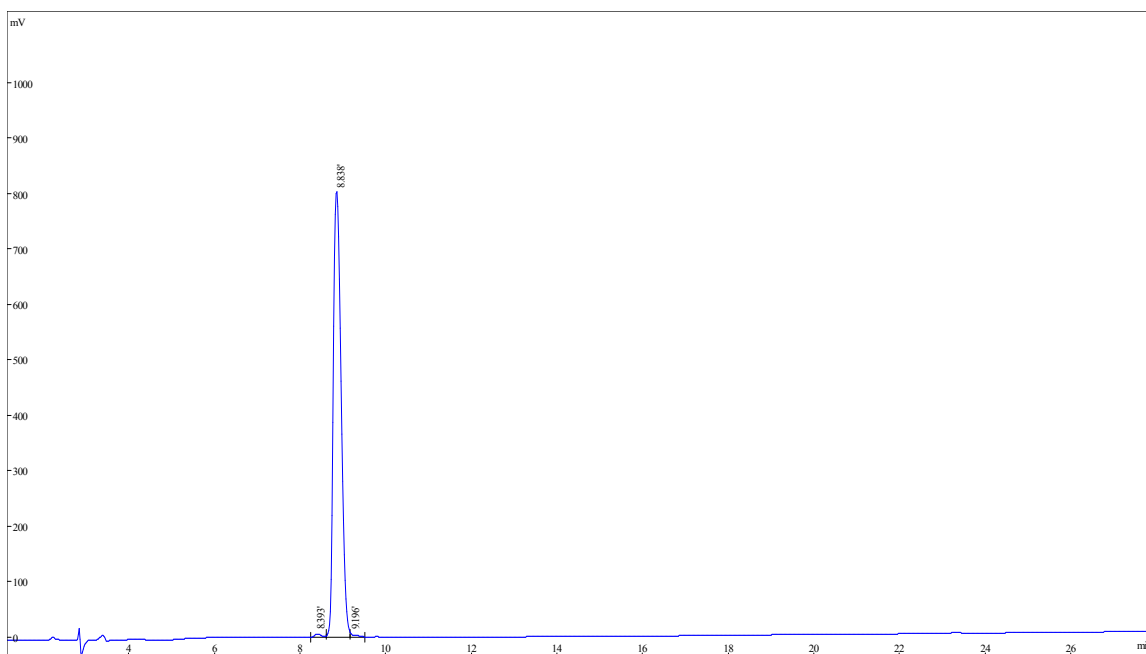

Number	Stay time	Concentration	Peak area	Peak height
1	8.393	0.6644	68589	6251
2	8.838	98.89	10209095	807695
3	9.196	0.4454	45978	4711
Total		100		