


## TB-500 HPLC

Test time	:05/07/2018, 10:27	Product Name	:TB-500
Analyst	:LZH	Batch number	:US20180507
Column	:GSA46250BI017013, C18, 4.6*250mm, 5um	Flow Rate	:1.0ml/min
Solvent A	:100% Acetonitrile	Wavelength	:220nm
Solvent B	:0.1% Trifluoroacetic in 100% Water	Temperature	:37°C
Gradient	:	Concentration	:1mg/ml
	A    B	Sample Volume	:10ul
	0.0min    5%    95%		
	25.0min    95%    5%		
	25.1min    100%    0%		
	30.0min    Stop		

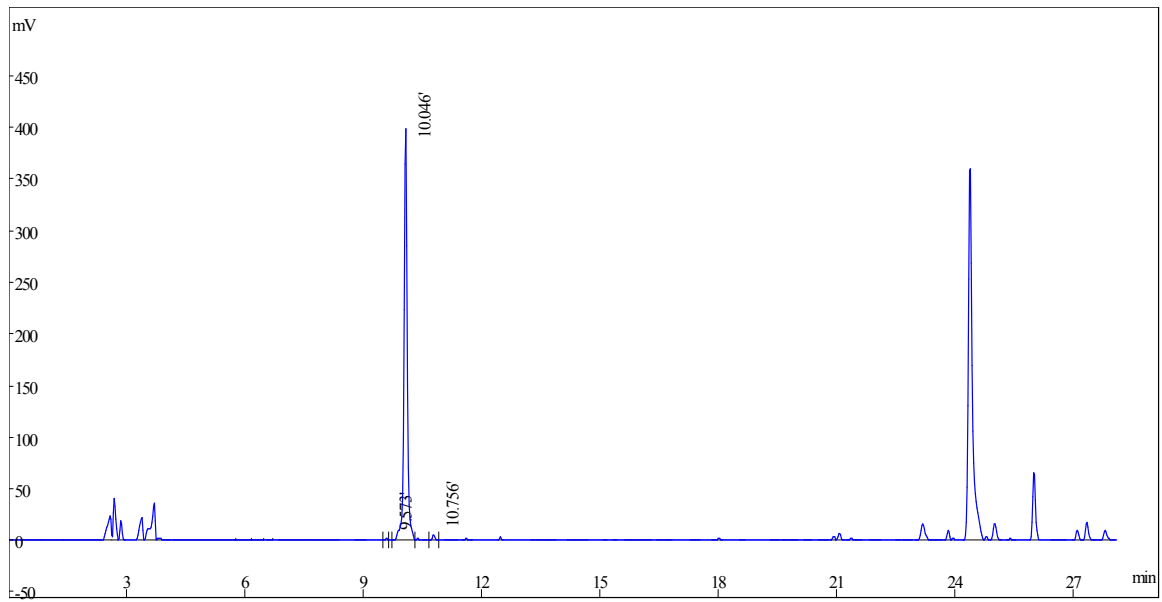

Number	Stay time	Concentration	Peak area	Peak height
1	9.573	0.2376	7805	2019
2	10.046	98.61	2275141	413165
3	10.756	1.1524	28875	6291
Total		100	2311821	421475